



FIG. 1

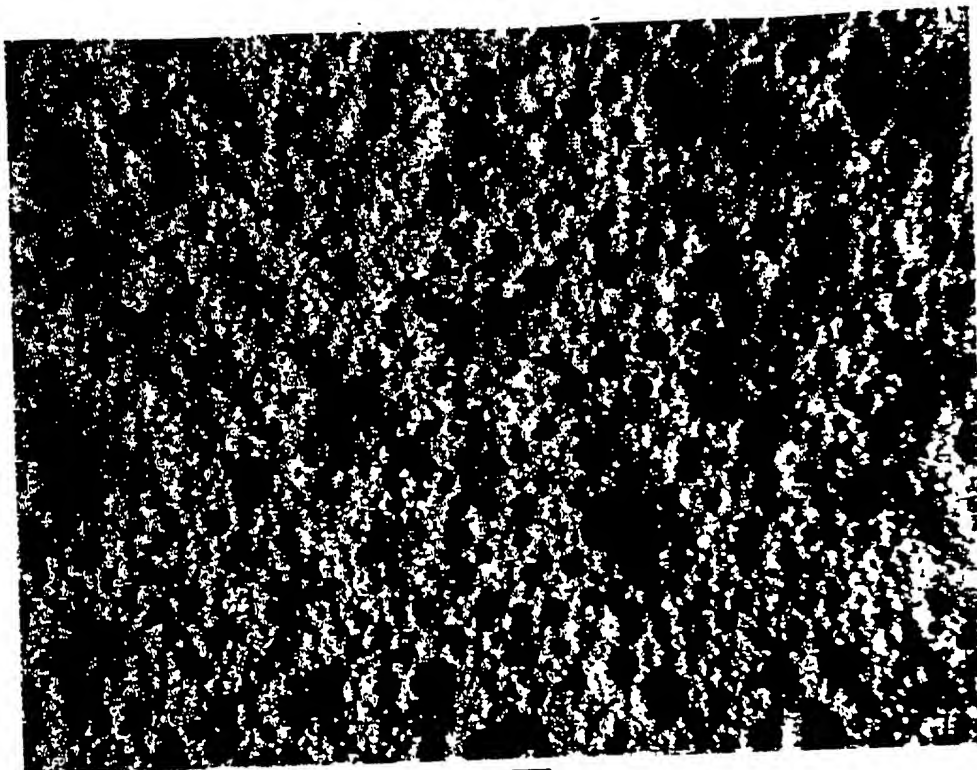

Injected Sample

1 millimeter


These two images were taken at the same magnification

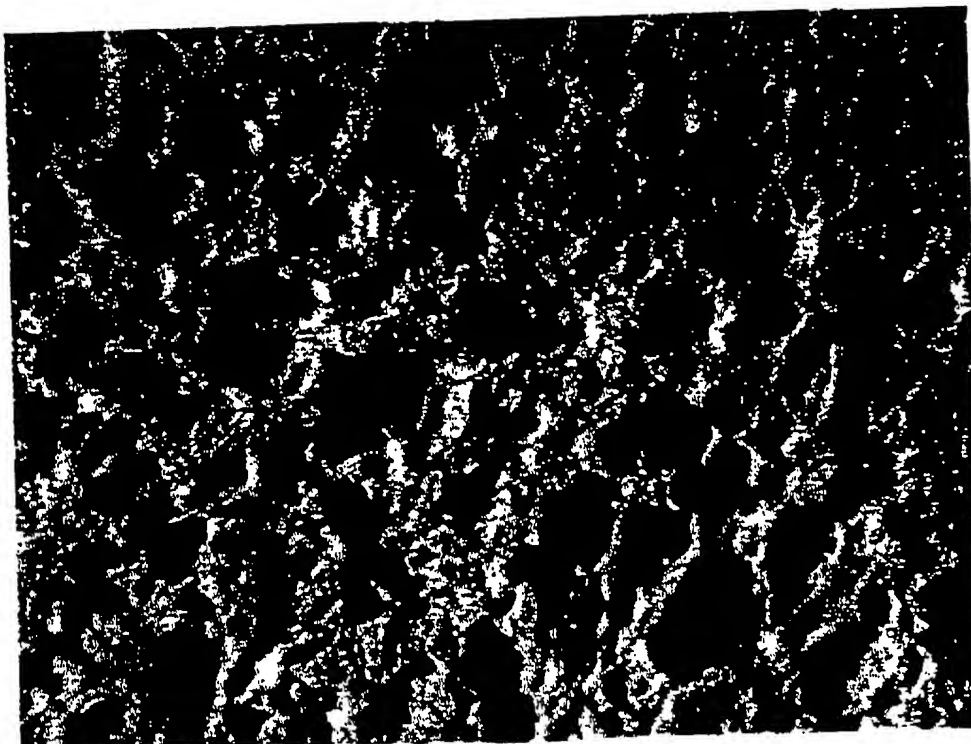

Uninjected Sample

1 millimeter

FIG. 2

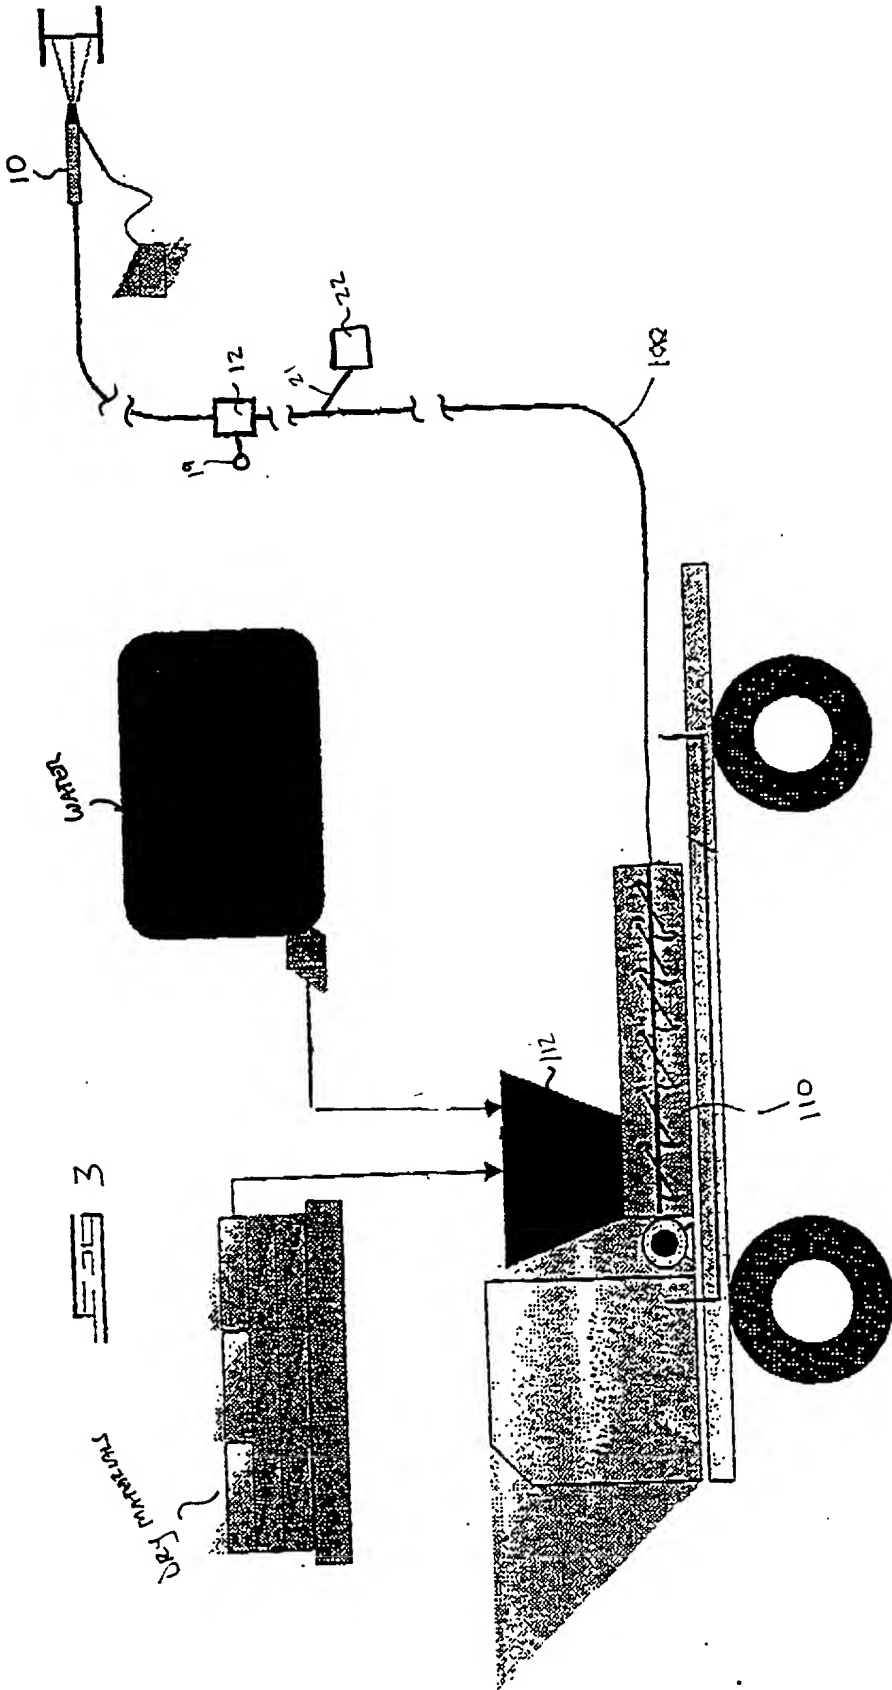

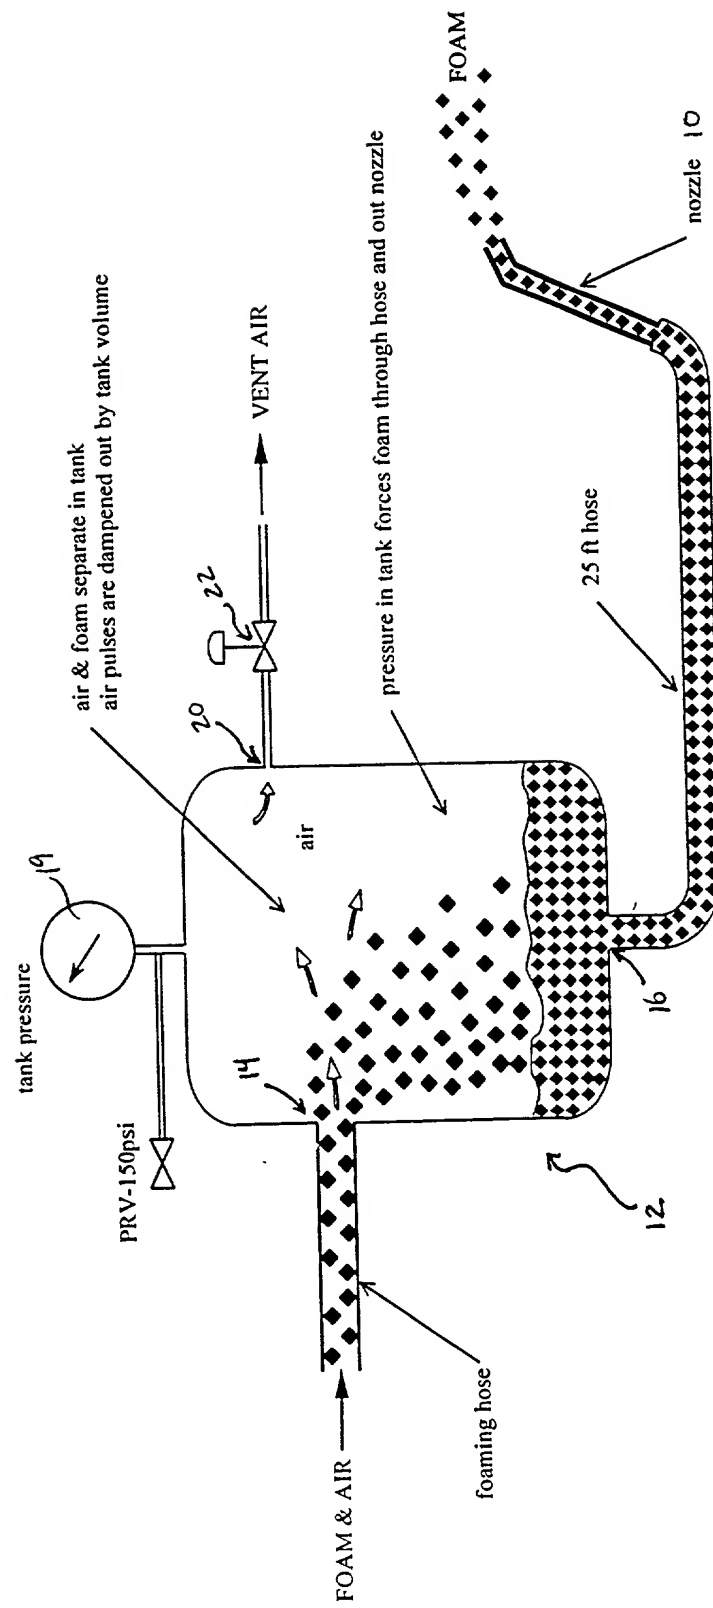


Fig. 4